

NAT'L INST OF STAND & TECH



111106 947810

NIST
PUBLICATIONS

REFERENCE

NIST Special Publication 260-164

Evaluation Specimens for Izod Impact Machines (SRM 2115): Report of Analysis

Tom Siewert
Jolene Splett
Ray Santoyo



QC
100
457
#260-164
2006

ST

National Institute of Standards and Technology • Technology Administration • U.S. Department of Commerce

The National Institute of Standards and Technology was established in 1988 by Congress to "assist industry in the development of technology ... needed to improve product quality, to modernize manufacturing processes, to ensure product reliability ... and to facilitate rapid commercialization ... of products based on new scientific discoveries."

NIST, originally founded as the National Bureau of Standards in 1901, works to strengthen U.S. industry's competitiveness; advance science and engineering; and improve public health, safety, and the environment. One of the agency's basic functions is to develop, maintain, and retain custody of the national standards of measurement, and provide the means and methods for comparing standards used in science, engineering, manufacturing, commerce, industry, and education with the standards adopted or recognized by the Federal Government.

As an agency of the U.S. Commerce Department's Technology Administration, NIST conducts basic and applied research in the physical sciences and engineering, and develops measurement techniques, test methods, standards, and related services. The Institute does generic and precompetitive work on new and advanced technologies. NIST's research facilities are located at Gaithersburg, MD 20899, and at Boulder, CO 80303. Major technical operating units and their principal activities are listed below. For more information visit the NIST Website at <http://www.nist.gov>, or contact the Publications and Program Inquiries Desk, 301-975-3058.

Office of the Director

- National Quality Program
- International and Academic Affairs

Technology Services

- Standards Services
- Technology Partnerships
- Measurement Services
- Information Services
- Weights and Measures

Advanced Technology Program

- Economic Assessment
- Information Technology and Applications
- Chemistry and Life Sciences
- Electronics and Photonics Technology

Manufacturing Extension Partnership Program

- Regional Programs
- National Programs
- Program Development

Electronics and Electrical Engineering

Laboratory

- Microelectronics
- Law Enforcement Standards
- Electricity
- Semiconductor Electronics
- Radio-Frequency Technology¹
- Electromagnetic Technology¹
- Optoelectronics¹
- Magnetic Technology¹

Materials Science and Engineering

Laboratory

- Intelligent Processing of Materials
- Ceramics
- Materials Reliability¹
- Polymers
- Metallurgy
- NIST Center for Neutron Research

Chemical Science and Technology

Laboratory

- Biotechnology
- Process Measurements
- Surface and Microanalysis Science
- Physical and Chemical Properties²
- Analytical Chemistry

Physics Laboratory

- Electron and Optical Physics
- Atomic Physics
- Optical Technology
- Ionizing Radiation
- Time and Frequency¹
- Quantum Physics¹

Manufacturing Engineering

Laboratory

- Precision Engineering
- Manufacturing Metrology
- Intelligent Systems
- Fabrication Technology
- Manufacturing Systems Integration

Building and Fire Research Laboratory

- Applied Economics
- Materials and Construction Research
- Building Environment
- Fire Research

Information Technology Laboratory

- Mathematical and Computational Sciences²
- Advanced Network Technologies
- Computer Security
- Information Access
- Convergent Information Systems
- Information Services and Computing
- Software Diagnostics and Conformance Testing
- Statistical Engineering

¹At Boulder, CO 80305

²Some elements at Boulder, CO

NIST Special Publication 260-164

Evaluation Specimens for Izod Impact Machines (SRM 2115): Report of Analysis

Tom Siewert

Ray Santoyo

*Materials Reliability Division
Materials Science and Engineering Laboratory*

Jolene Splett

*Statistical Engineering Division
Information Technology Laboratory*

*National Institute of Standards and Technology
Boulder, Colorado 80305*

October 2006



U.S. Department of Commerce

Carlos M. Gutierrez, Secretary

Technology Administration

Robert Cresanti, Under Secretary of Commerce for Technology

National Institute of Standards and Technology

William A. Jeffrey, Director

Certain commercial entities, equipment, or materials may be identified in this document in order to describe an experimental procedure or concept adequately. Such identification is not intended to imply recommendation or endorsement by the National Institute of Standards and Technology, nor is it intended to imply that the entities, materials, or equipment are necessarily the best available for the purpose.

National Institute of Standards and Technology Special Publication 260-164
Natl. Inst. Stand. Technol. Spec. Publ. 260-164, 10 pages (October 2006)
CODEN: NSPUE2

U.S. GOVERNMENT PRINTING OFFICE
WASHINGTON: 2006

For sale by the Superintendent of Documents, U.S. Government Printing Office
Internet: bookstore.gpo.gov — Phone: (202) 512-1800 — Fax: (202) 512-2250
Mail: Stop SSOP, Washington, DC 20402-0001

Contents

1. Introduction.....	1
2. Experimental Design and Analysis.....	3
3. Material Homogeneity	5
4. Reference Value and Uncertainty	5
5. Discussion	6
6. References	7

Evaluation Specimens for Izod Impact Machines (SRM 2115): Report of Analysis

Tom Siewert,* Jolene Splett,[†] and Ray Santoyo*

National Institute of Standards and Technology
325 Broadway
Boulder, CO 80305

In the past few years, we have received a number of requests to verify the performance of Izod impact machines, similar to what we offer for Charpy impact machines. Although there are similarities between Izod and Charpy impact testing, there are some notable differences that needed to be examined, including test temperature (the Izod configuration precludes cooling), specimen orientation, and specimen length. This report describes the development of a final Izod specimen design and test procedure, that produced a suitable mean energy and a coefficient of variation similar to what is found in the Charpy program.

Keywords: impact test; Izod impact; standard reference materials

1. Introduction

ASTM Standard E23, “Standard Test Methods for Notched Bar Impact Testing of Metallic Materials” (Ref. [1]) describes procedures for pendulum impact testing in both Charpy and Izod configurations. It is most commonly used with the Charpy specimen configurations, and most users are familiar with verification procedures. However, Standard E23 offers no guidelines for verification of Izod machine performance by test specimens. In fact, there are no known sources for Izod verification specimens from any national measurement institute around the world. This report describes the development of such specimens in two steps: (1) investigation of the effects of the differences between the Izod and Charpy configurations, and (2) characterization of the Izod specimens to a degree where they could be used to verify the performance of Izod impact machines.

*Materials Reliability Division
Materials Science and Engineering Laboratory

[†]Statistical Engineering Division
Information Technology Laboratory

Figure 1 shows a Charpy impact specimen (on the left) and an Izod specimen (on the right). Both specimens have an identical cross section (10 mm by 10 mm) and an identical V notch (located 27.5 mm from one end for Charpy specimens and 28 mm from one end for Izod specimens). Figure 1 also shows a substantial difference in their overall length (55 mm for Charpy and 75 mm for Izod) due to the end clamp design of the Izod configuration.

NIST offers Charpy impact specimens in a variety of energies (from near 15 J to 200 J) that are designed to span the capacity range of most impact machines. For the initial evaluation of Izod machines, we decided to start with a single energy range, and selected the material used in the low-energy range for Charpy machines (SRM 2092). The material is heat treated to the highest strength, so it has a high resistance to fracture but for only a short period of time (Ref. [2]), which produces a fairly low absorbed energy value, near 15 J on a Charpy machine. As the force must be counterbalanced by the machine, this sharp blow also translates to a quick shock load to the machine anvil and striker, an effective, yet simple evaluation of the quality of the machine and its mounts. However, the Izod test procedure requires aligning and clamping the specimen in an Izod vise (a relatively slow process), and so this necessitates testing at room temperature, instead of the $-40\text{ }^{\circ}\text{C}$ temperature used for the SRM 2092 Charpy procedure. This upward shift in temperature was expected to raise the absorbed energy slightly, and is one example of the procedural changes that needed to be evaluated.



Figure 1. Photograph comparing a Charpy specimen (left) and Izod specimen (right).

2. Experimental Design and Analysis

A group of Izod specimens was machined and heat treated along with one of our standard batches of low-energy Charpy reference specimens (LL104), using the same shop and steel. The specimens were all tested at the same time, in the NIST Charpy reference laboratory by the same technician. Standard Charpy specimens will fit in an Izod machine, but not vice versa. Thus, we decided to test all feasible combinations of specimens and machines to validate the Izod results. Data were collected *at room temperature* for the two kinds of specimens, Izod and Charpy, as follows.

1. A NIST Charpy reference machine was used to test five Charpy specimens. (Charpy/Charpy)
2. A NIST Izod machine was used to test five Charpy specimens. (Izod1/Charpy)
3. A NIST Izod machine was used to test 25 Izod specimens. (Izod1/Izod)
4. An *external* Izod machine was used to test 10 Izod specimens. (Izod2/Izod)

The raw data are shown in Figure 2 for each of the four machine/specimen combinations, or treatment groups.

Visual inspection of the raw data indicates that there is greater variation in measurements obtained with the NIST Izod machine than measurements obtained with the NIST Charpy machine, regardless of specimen type. In addition, the data points do not overlap at all for

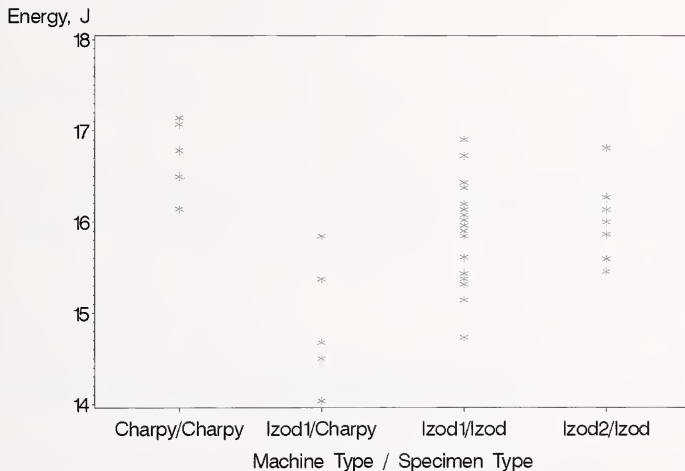


Figure 2. Measurement results for four treatment groups. Some test results are nominally the same, so not all data points are visible on the graph.

Charpy/Charpy and Izod1/Charpy treatment groups. The apparent discrepancy between the two NIST machines (Charpy and Izod1) can be attributed to the difference in toss energy, as only one end of the specimen is free to move as the specimen is struck in the Izod configuration. The possible shift in data means between Charpy specimens tested in the NIST Izod machine to Izod specimens tested in the NIST Izod machine might be at least partially explained by a change in stiffness between the two specimens in the Izod mount. The external Izod machine appears to agree with the NIST Izod machine fairly well. The values for Charpy specimens tested on the Charpy machine at room temperature were several joules higher than the certified value of LL104 (tested at $-40\text{ }^{\circ}\text{C}$), a quite reasonable and expected difference. Figure 3 displays group means along with error bars ($\pm 2s_i/\sqrt{n_i}$).

A one-way analysis of variance to compare group means indicates that at least one mean is different from the others (p value <0.0001). Next, we compared each group to Izod1/Izod separately to determine whether other treatment groups can validate the Izod1/Izod results. Table 1 displays the results of the comparisons of the individual treatment groups.

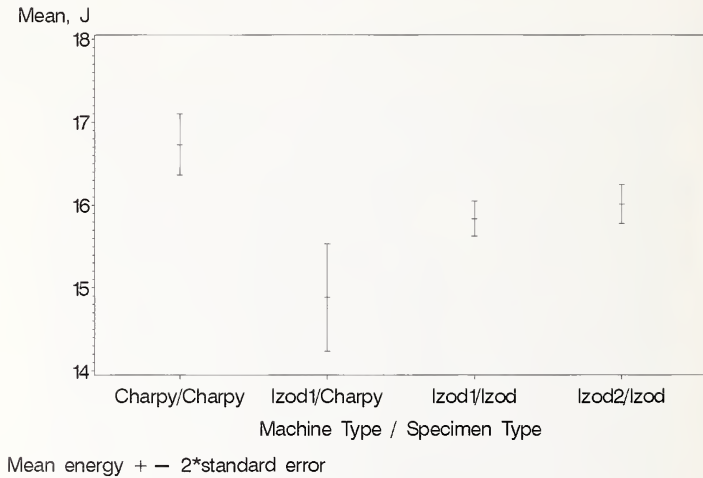


Figure 3. Treatment group means with error bars. The error bars are twice the standard error of the mean.

Table 1. Pairwise comparisons of treatment group means.

Parameter	Estimate, J	Stand. error, J	t Value	Pr > t
Charpy/Charpy – Izod1/Izod	0.893	0.249	3.59	0.0009
Izod1/Charpy – Izod1/Izod	-0.950	0.249	-3.82	0.0004
Izod2/Izod – Izod1/Izod	0.176	0.190	0.93	0.4

Table 2. Summary statistics for Izod data.

	Izod machine #1 - NIST	Izod machine #2 - External
n_i	25	10
\bar{x}_i	15.836 J	16.012 J
s_i	0.522 J	0.375 J
$u(\bar{x}_i) = \bar{s}_i / \sqrt{n_i}$	0.104 J	0.119 J
ν_i	24	9

The analysis indicates that the means of the Izod1/Izod and Izod2/Izod treatment groups do not differ significantly. However, the means for both Charpy/Charpy and Izod1/Charpy treatment groups differ significantly from Izod1/Izod. Thus, only the Izod2/Izod data can be used to confirm the Izod1/Izod data. The Charpy specimens measured on the NIST Izod machine do not (and were not expected to) validate the Izod1/Izod measurements, but do show the differences between (a) Izod specimens tested in an Izod machine, and (b) Charpy specimens in an Izod machine or Charpy specimens in a Charpy machine.

3. Material Homogeneity

The manufacturing process for Izod specimens was identical to that for Charpy specimens, the only difference being that the Izod specimens were machined to slightly different dimensional specifications than those of Charpy specimens. Thus, the batch of Izod specimens is considered to be fairly homogeneous, based on past experience with specimens manufactured for the Charpy verification program.

4. Reference Value and Uncertainty

Table 2 displays the information necessary to compute the reference value and its associated uncertainty for batch LL104 of Izod SRM specimens.

The measurement equation used to determine the reference value is

$$Y = X + B,$$

where $X = \bar{x}_1 = 15.836$ J is the mean of the 25 measurements of Izod specimens taken on the NIST Izod machine, and B is an unknown bias that has a Type B rectangular distribution centered about zero. The reference value is

$$Y = X + B = 15.836 + 0 = 15.836 \text{ J.}$$

We used a method called BOB (Type B on Bias) to compute the uncertainty of the reference value using the NIST Izod within-machine variation and the variation between the two Izod machines. (See Ref. [3] for details regarding the BOB method.)

The within-machine uncertainty, $u(X) = u(\bar{x}_1) = 0.104$ J, was computed using the 25 measurements on the NIST Izod machine and has $\nu_X = \nu_1 = 24$ degrees of freedom.

The between-machine uncertainty $u(B)$ and associated degrees of freedom ν_B ,

$$u(B) = \frac{|\bar{x}_1 - \bar{x}_2|}{2\sqrt{3}} = \frac{|15.836 - 16.012|}{2\sqrt{3}} = 0.051 \text{ J, and}$$

$$\nu_B = \frac{\frac{1}{2}(\bar{x}_2 - \bar{x}_1)^2}{u^2(\bar{x}_1) + u^2(\bar{x}_2)} = 0.62 \Rightarrow 1,$$

were computed based on the rectangular Type B distribution.

The combined standard uncertainty of the reference value is

$$u_c(Y) = \sqrt{u^2(X) + u^2(B)} = \sqrt{(0.104)^2 + (0.051)^2} = 0.116 \text{ J.}$$

The Satterthwaite approximation (Ref. [4]) was used to compute the effective degrees of freedom as follows:

$$\nu_c = \frac{u_c^4(Y)}{\frac{u^4(X)}{\nu_X} + \frac{u^4(B)}{\nu_B}} = \frac{(0.116)^4}{\frac{(0.104)^4}{24} + \frac{(0.051)^4}{1}} = 15.5 \Rightarrow 15.$$

Thus, the expanded uncertainty associated with a 95 % confidence interval is

$$U = t_{0.975,15}(u_c) = 2.131(0.116) = 0.247 \text{ J.}$$

5. Discussion

The results presented in this document indicate that an Izod machine verification program similar to that for Charpy machines is feasible. We developed appropriate test methods and validated the NIST Izod measurement results with a secondary Izod machine. We computed a reference value and its associated uncertainty. The data for the two Izod machines agree well, but Izod data do not agree with Charpy data, even when specimens are produced from the same batch of material. This disagreement may be due to inherent differences between the two types of machines, such as, for example, differences in toss energy for the two machines.

6. References

- [1] ASTM Standard E23, Standard test methods for notched bar impact testing of metallic materials, ASTM International, West Conshohocken, Pennsylvania (2005).
- [2] C. N. McCowan, T. A. Siewert, and D. P. Vigliotti, Charpy verification program: Reports covering 1989–2002, NIST Technical Note 1500-9 (September 2003), p. 10.
- [3] Levenson, M. S., Banks, D. L., Eberhardt, K. R., Gill, L. M., Guthrie, W. F., Liu, H. K., Vangel, M. G., Yen, J. H., and Zhang, N. F., An approach to combining results from multiple methods motivated by the ISO GUM, NIST Journal of Research 105(4): 571-579 (July–August 2000).
- [4] B. N. Taylor and C. E. Kuyatt, Guidelines for evaluating and expressing uncertainty in NIST measurement results, NIST Technical Note 1297 (1994).

NIST Technical Publications

Periodical

Journal of Research of the National Institute of Standards and Technology—Reports NIST research and development in metrology and related fields of physical science, engineering, applied mathematics, statistics, biotechnology, and information technology. Papers cover a broad range of subjects, with major emphasis on measurement methodology and the basic technology underlying standardization. Also included from time to time are survey articles on topics closely related to the Institute's technical and scientific programs. Issued six times a year.

Nonperiodicals

Monographs—Major contributions to the technical literature on various subjects related to the Institute's scientific and technical activities.

Handbooks—Recommended codes of engineering and industrial practice (including safety codes) developed in cooperation with interested industries, professional organizations, and regulatory bodies.

Special Publications—Include proceedings of conferences sponsored by NIST, NIST annual reports, and other special publications appropriate to this grouping such as wall charts, pocket cards, and bibliographies.

National Standard Reference Data Series—Provides quantitative data on the physical and chemical properties of materials, compiled from the world's literature and critically evaluated. Developed under a worldwide program coordinated by NIST under the authority of the National Standard Data Act (Public Law 90-396). NOTE: The Journal of Physical and Chemical Reference Data (JPCRD) is published bimonthly for NIST by the American Institute of Physics (AIP). Subscription orders and renewals are available from AIP, P.O. Box 503284, St. Louis, MO 63150-3284.

Building Science Series—Disseminates technical information developed at the Institute on building materials, components, systems, and whole structures. The series presents research results, test methods, and performance criteria related to the structural and environmental functions and the durability and safety characteristics of building elements and systems.

Technical Notes—Studies or reports which are complete in themselves but restrictive in their treatment of a subject. Analogous to monographs but not so comprehensive in scope or definitive in treatment of the subject area. Often serve as a vehicle for final reports of work performed at NIST under the sponsorship of other government agencies.

Voluntary Product Standards—Developed under procedures published by the Department of Commerce in Part 10, Title 15, of the Code of Federal Regulations. The standards establish nationally recognized requirements for products, and provide all concerned interests with a basis for common understanding of the characteristics of the products. NIST administers this program in support of the efforts of private-sector standardizing organizations.

Order the following NIST publications—FIPS and NISTIRs—from the National Technical Information Service, Springfield, VA 22161.

Federal Information Processing Standards Publications (FIPS PUB)—Publications in this series collectively constitute the Federal Information Processing Standards Register. The Register serves as the official source of information in the Federal Government regarding standards issued by NIST pursuant to the Federal Property and Administrative Services Act of 1949 as amended, Public Law 89-306 (79 Stat. 1127), and as implemented by Executive Order 11717 (38 FR 12315, dated May 11, 1973) and Part 6 of Title 15 CFR (Code of Federal Regulations).

NIST Interagency or Internal Reports (NISTIR)—The series includes interim or final reports on work performed by NIST for outside sponsors (both government and nongovernment). In general, initial distribution is handled by the sponsor; public distribution is handled by sales through the National Technical Information Service, Springfield, VA 22161, in hard copy, electronic media, or microfiche form. NISTIR's may also report results of NIST projects of transitory or limited interest, including those that will be published subsequently in more comprehensive form.

U.S. Department of Commerce
National Bureau of Standards and Technology
325 Broadway
Boulder, CO 80305-3328

Official Business
Penalty for Private Use \$300